


*Difference between spectra at the field locations; the spectrum at the center of the field (leftmost in second row below) is taken as reference*

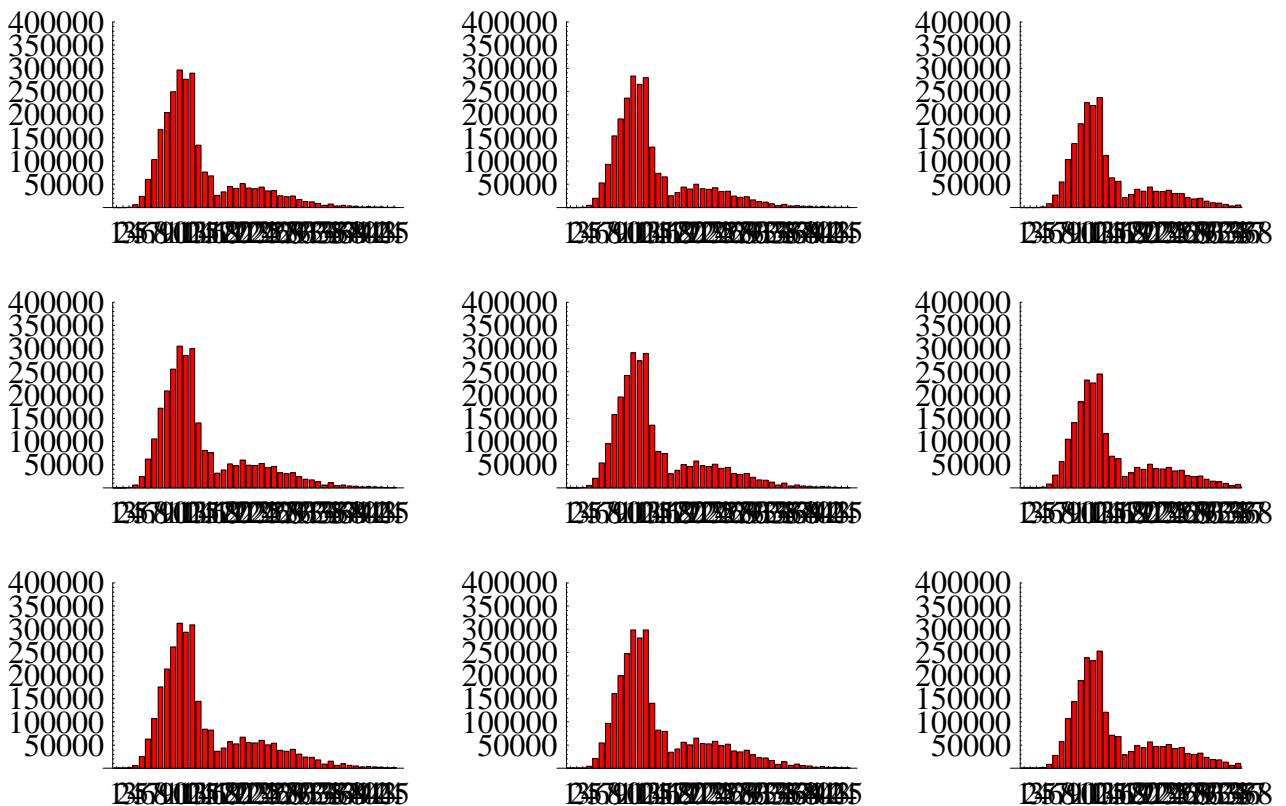

*Spectra computed at the field locations. First row is top of scan (+25mm), lowest bottom of scan (-25mm). Left column is field center, rightmost is +25mm field position.*